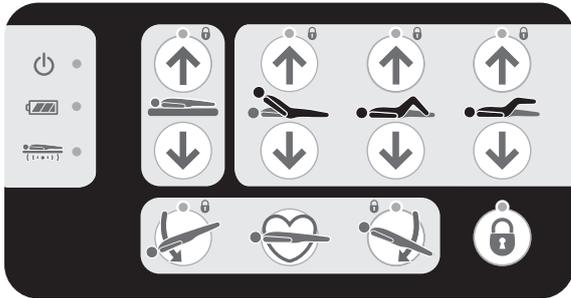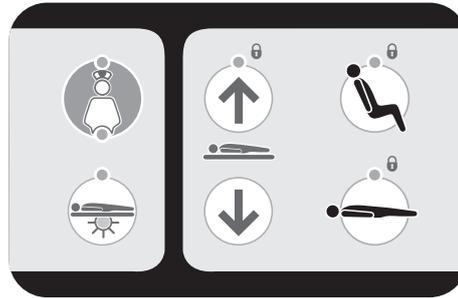# Citadel Plus

CE 2797

## Attendant Control Panel



## Nurse Control Panel



## Patient Handset



## Patient Control Panel
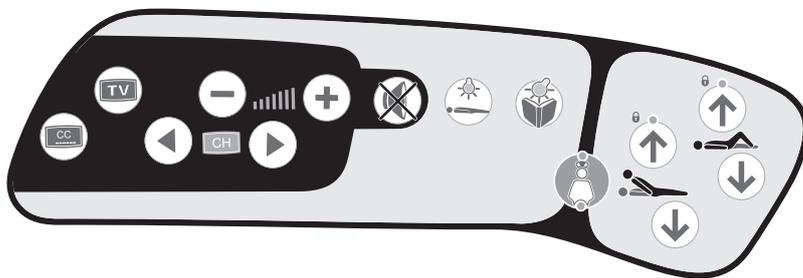


 ● **Power On Indicator**

 ● **Battery Status LED Indicator**

| | | |
|---|---|---|
|  | ● | Battery fully charged |
|  | 🟡 | Battery charging |
|  | 🔴 | Battery discharged |

**Anti-Entrapment System (AES) Indicator** - When illuminated, AES system has been activated and obstruction needs to be removed before the frame will lower.

**Mattress Platform Height** - Raise or lower the mattress platform.

**Backrest Angle** - Raise or lower the backrest.

**Thigh Section** - Raise or lower the thigh section.

**Calf Section** - Raise or lower the calf section.

**Lower head end** (Trendelenburg position)

**Lower foot end** (Reverse Trendelenburg position)

**CPR Position** - Flattens the mattress platform and lowers the bed height

**Function Lockout** - Press the button, then press selected Attendant Control Panel button(s) to lock or unlock function. Yellow light = locked.

arjo

*with people in mind*

**Auto-Chair**

(nurse control panel only) - Press and hold for chair position.

**Auto-Chair Down**

(nurse control panel only) - Press and hold to return to flat level position.

**Under Bed Light**

(nurse control panel only)

**Nurse Call**

(available on selected models) - Press to request assistance.

**Reading lamp**

(available on selected models)- Press to turn on light.

**Reading lamp on/off**

(available on selected models)

**Sound on/off (mute)**

(available on selected models)

**Volume down**

(available on selected models)

**Volume up**

(available on selected models)

**Channel down**

(available on selected models)

**Channel up**

(available on selected models)
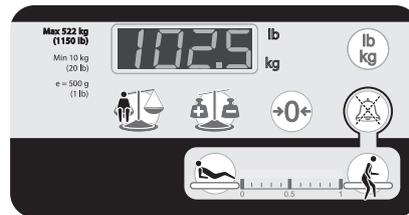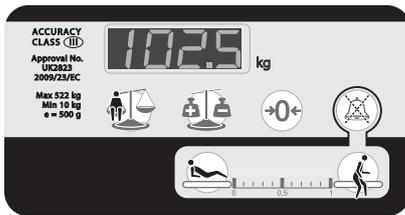
**Television on/off**

(available on selected models)

**Closed caption on/off**

(available on selected models)

## Weigh Scale Control Panel

**Zero** - Press to reset weighing system when bed is first set up and before a new patient is placed on the bed.

**Auto Compensation** - Press when adding or removing items from the bed without affecting the indicated patient weight.

**Weigh** - Press to display weight.

**Select Units** - Press to select weighing unit.

**VariZone Mute Button** - Press to mute exit alarm for three minutes.

**Patient movement detection threshold** - An indicator shows the selected sensitivity of patient movement.

**In Bed** - Press to reactivate or activate patient movement detection and increase sensitivity.

**Egress** - Press to reactivate or activate patient movement detection and decrease sensitivity.

**arjo**

*with people in mind*